

A New Ozone Concentration Regulator

Michael David, Tay Ching En Marcus, Maslina Yaacob, Mohd Rashidi Salim,
Nabihah Hussin, Mohd Haniff Ibrahim*, Sevia Mahdaliza Idrus, Nor Hafizah Ngajikin,
Asrul Izam Azmi

Lightwave Communication Research Group, Infocomm Research Alliance,
Faculty of Electrical Engineering, Universiti Teknologi Malaysia, 81310 Skudai, Johor, Malaysia
*Corresponding author, e-mail: ahanif@fke.utm.my, bsevia@fke.utm.my, am david2@live.utm.my
hanif@fke.utm.my, mdavid2@live.utm.my

Abstract

Laboratory design of an ozone concentration regulator which is build on the theory of continuity equation for gas flow in parallel pipes in conjunction with the ozone elimination potentials of an ozone destructor is presented. At an initial oxygen flow rate of $33.33 \text{ cm}^3\text{s}^{-1}$, ozone concentration was generated and varied between 429.30 parts per million (ppm) to 3826.60 ppm. Similarly at an initial oxygen flow rate of $25 \text{ cm}^3\text{s}^{-1}$, ozone concentration was generated and varied between 387.30 ppm to 4435.20 ppm. Effect of flow meter when the ozone concentration was set to approximate 1000 ppm were investigated and reported. Fine tuning of the regulator is necessary to ensure concentration stability for long duration experimental work.

Keywords: flow rate, continuity, variable concentration, regulator, internal radius

Copyright © 2015 Institute of Advanced Engineering and Science. All rights reserved.

1. Introduction

Ozone application is diverse [1-8] and the requirement for each application differs from the other in terms of the required quantity. Ozone generators whose outputs are proportional to the oxygen or air flow rate input, generates very high amount of ozone at a low flow rates [9, 10]. The higher the oxygen or air flow rate the lower the amount of ozone generated and vice versa [9]. Thus, it is difficult or almost impossible to obtained lower concentrations at lower flow rates of air or oxygen. Investigation of sensing parameters such as response time which is more pronounced at lower flow rates becomes difficult at lower concentrations [11-14]. In this work we have designed and developed a laboratory based ozone concentration variable regulator which transforms a fixed ozone output generator into a variable concentration generator with available laboratory equipments and thus expanding the capability and applications of an ozone generator such that when ozone is generated at a low flow rate, varying concentrations can be obtained by means of the variable output regulator.

2. Theoretical Background and Regulator Design

When a gas flow in a parallel network of pipes as depicted in Figure 1, by continuity [15] the volume rate of discharge Q (cm^3/s) is express as:

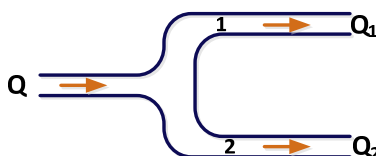


Figure 1. Flow in a parallel network of pipes

$$Q = Q_1 + Q_2 \quad (1)$$

Where:

$$Q = \frac{V}{t} = \frac{\pi r^2 L}{t} \quad (2)$$

$$Q_1 = \frac{\pi r_1^2 L_1}{t_1} \quad (3)$$

$$Q_2 = \frac{\pi r_2^2 L_2}{t_2} \quad (4)$$

Q = Volume rate of discharge (cm^3/s)

Q_1 = Volume rate of discharge in section 1 (cm^3/s)

Q_2 = Volume rate of discharge in section 2 (cm^3/s)

V = Volume of gas with volume rate of discharge of Q (cm^3)

V_1 = Volume of gas in section 1 (cm^3)

V_2 = Volume of gas in section 2 (cm^3)

r = radius of pipe section with volume rate of discharge of Q (cm)

r_1 = radius of pipe section 1 (cm)

r_2 = radius of pipe section 2; for our design $r_2 = 0.3\text{cm}$

L = length of pipe section with volume rate of discharge of Q (cm)

L_1 = length of pipe section 1; for our design $L_1 = 45.5\text{ cm}$

L_2 = length of pipe section 2; for our design $L_2 = 97.5\text{ cm}$

t = time (s)

t_1 = time of flow in section 1 (s)

t_2 = time of flow in section 2 (s)

From equation (1) to (4) above:

$$Q_1 = Q - Q_2$$

$$Q_1 = Q - \frac{\pi r_2^2 L_2}{t_2} = Q - \frac{\pi \times r_2^2 \times 97.5}{t_2} \quad (5)$$

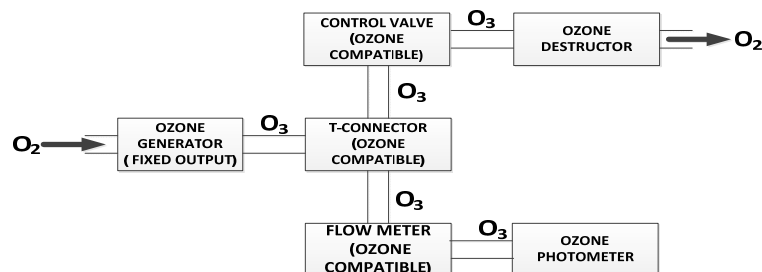


Figure 2. Block diagram of ozone concentration regulator

Q_1 or Q_2 depends on the level of freedom or resistance to gas flow which is proportional to the length and internal radius of the respective pipes [16]. In equation 5, when Q , r_1 , L_1 , L_2 and t_2 are kept constant; variation of the radius r_2 (between 0 and 0.3 cm) will produce a corresponding variation in the amount of flow both through sections 1 and 2 of Figure 1 and thereby varying the value of Q_1 and thus controlling the concentration in the different sections of the system [15]. The implementation of the said control for ozone gas is described in the block diagram of Figure 2. At lower concentrations requirements, excess ozone produced is eliminated by flowing it through an ozone destructor.

3. Experimental Set-up and Procedure

Figure 3 shows the experimental setup of our ozone regulator incorporated to an ozone photometer. The items in Figure 3 are described as follows: (1) Ozone destructor made in the

US by Longevity Resources Inc; (2) A silicon tube connecting a control valve to the ozone destructor; (3) A control valve that varies the flow of ozone gas to the destructor; (4) A silicone tube connecting the control valve and a T-connector; (5) Ozone compatible T-connector; (6) - A silicone tube connecting the T-connector to a flow meter; (7) A silicone tube connecting a ozone generator output into the T-connector; (8) EXT50 Ozone generator made in the US by Longevity Resources Inc; (9) Vinyl tube for connecting the flow of oxygen from the oxygen tank to the ozone generator; (10) 220V electricity supply to the ozone generator; (11) 0 to 10 LPM (0 to $166.67 \text{ cm}^3\text{s}^{-1}$) ozone compatible flow meter; (12) A silicone tube connecting the flow meter to ozone monitor; (13) 2B technologies 106-M model ozone monitor which can measure accurate ozone concentrations between 0 to 1000 ppm; (14) USB cable connecting the monitor to a laptop computer and (15) A DC source to power the ozone monitor.

Oxygen gas with a purity of 99.999% was delivered at a flow rate of $33.33 \text{ cm}^3\text{s}^{-1}$ [2 liters per minute (LPM)] through a vinyl tubing to the EXT50 Ozone generator. Ozone was generated and fed into the ozone monitor at a flow rate of $33.33 \text{ cm}^3\text{s}^{-1}$. The control valve was completely locked so that there was no flow of ozone gas to the ozone destructor.

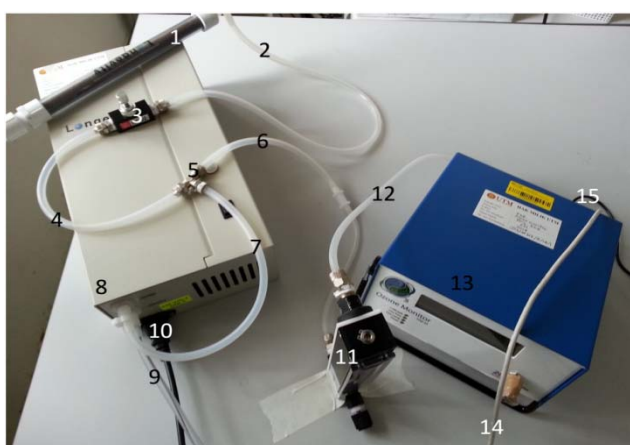


Figure 3. Experimental setup of an ozone concentration regulator

The ozone concentration in ppm were extracted from the monitor through the USB connection to the laptop. With the ozone gas flowing at a rate of $33.33 \text{ cm}^3\text{s}^{-1}$, the control valve was completely opened and ozone flowed into the destructor and the corresponding effect on the flow rate and the concentration were noted and recorded. With the aid of the control valve, the ozone concentration was adjusted to approximately 1000 ppm which corresponds to a flow rate of approximately $30.00 \text{ cm}^3\text{s}^{-1}$ (1.8 LPM). The effect of the flow meter on this adjusted concentration of 1000 ppm was then investigated for a flow rate between $16.67 \text{ cm}^3\text{s}^{-1}$ (1LPM) and $166.67 \text{ cm}^3\text{s}^{-1}$ (10 LPM) at a step of $16.67 \text{ cm}^3\text{s}^{-1}$ or 1LPM. The entire process was repeated for an initial oxygen flow rate of $25 \text{ cm}^3\text{s}^{-1}$ (1.5 LPM) and the results were obtained and analysed.

4. Results and Discussion

Figure 4 shows the maximum and minimum ozone concentrations in ppm obtained at an initial oxygen flow rate of $33.33 \text{ cm}^3\text{s}^{-1}$ (Initial oxygen flow rate is the flow rate of oxygen in the system before the ozone generator was energised electrically). The section 'A' is when oxygen was fed into the ozone generator while the ozone generator was off.

B indicates the maximum ozone concentrations 3826.60 ppm at an initial oxygen flow rate of $33.33 \text{ cm}^3\text{s}^{-1}$ with the control valve completely locked to short out ozone from the destructor. C is the lowest ozone concentration obtained 429.30 ppm, when the control valve was completely opened thus allowing maximum flow of ozone to the destructor. Thus, the percentage regulation at a flow rate of $33.33 \text{ cm}^3\text{s}^{-1}$ is in the range of 11.22% to 100%.

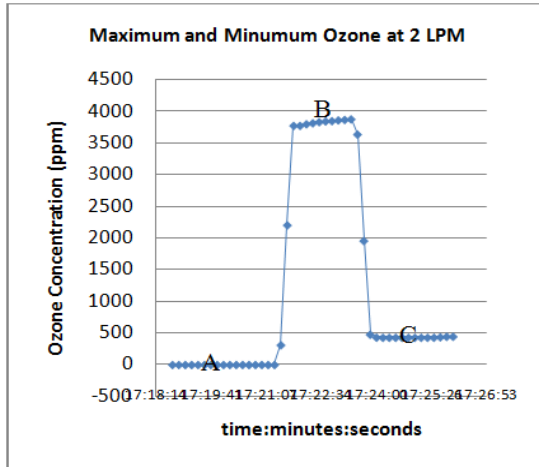


Figure 4. Maximum and minimum ozone concentrations at an oxygen flow rate of $33.33\text{cm}^3\text{s}^{-1}$ (2 LPM)

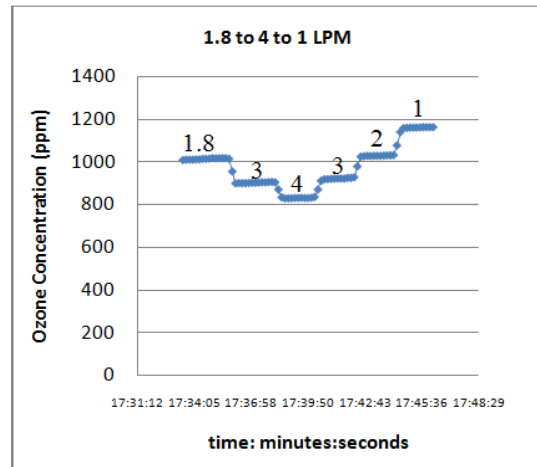


Figure 5. Effect of flow meter between $30\text{cm}^3\text{s}^{-1}$ to $66.67\text{cm}^3\text{s}^{-1}$ to $16.67\text{cm}^3\text{s}^{-1}$ (1.8 to 4 to 1 LPM) of ozone concentrations

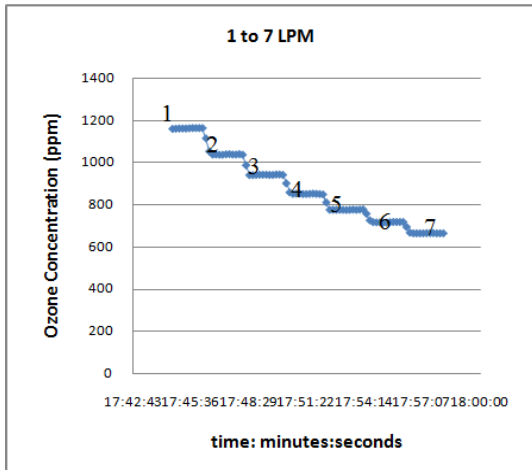


Figure 6. Effect of flow meter between $16.67\text{cm}^3\text{s}^{-1}$ and $116.67\text{cm}^3\text{s}^{-1}$ (1 and 7 LPM) of ozone concentrations

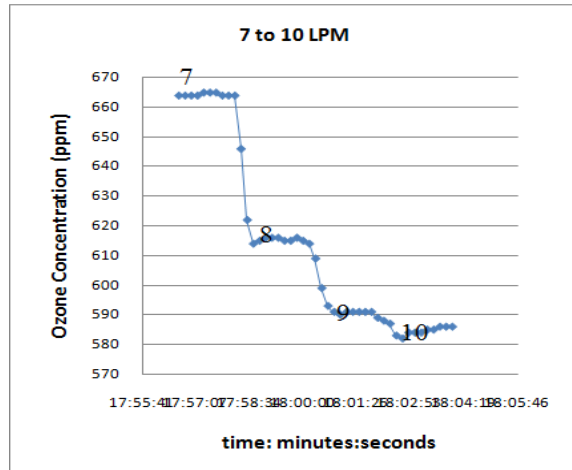


Figure 7. Effect of flow meter between $116.67\text{cm}^3\text{s}^{-1}$ and $166.67\text{cm}^3\text{s}^{-1}$ (7 and 10 LPM) of ozone concentrations

In Figure 5, 6, 7 and 8 the effect of the flow meter when the ozone was set to 1000 ppm approximately is shown. The concentrations in ppm obtained for ozone flow rate of $16.67\text{cm}^3\text{s}^{-1}$ to $166.67\text{cm}^3\text{s}^{-1}$ (1 to 10 LPM) respectively are 1163.60, 1039.20, 942.50, 776.10, 716.70, 664.30, 615.20, 590.60 and 584.50 ppm. Thus the higher the flow rate the lower the concentrations, this is depicted clearly in Figure 9. Figure 10 is the fluctuations in pressure at higher flow rates, which shows that the regulator is effective between $16.67\text{cm}^3\text{s}^{-1}$ to $116.67\text{cm}^3\text{s}^{-1}$ (1 to 7 LPM) since the pressure is not longer able to sustain a steady flow as from 8 LPM upwards. This can also viewed in Figure 7. At D in Figure 8, the ozone generator is switched off and ozone concentration becomes reduced to approximately zero. The results thus obtained are in agreement with the theory of gas flow in parallel pipes as earlier shown in section 2 of this article.

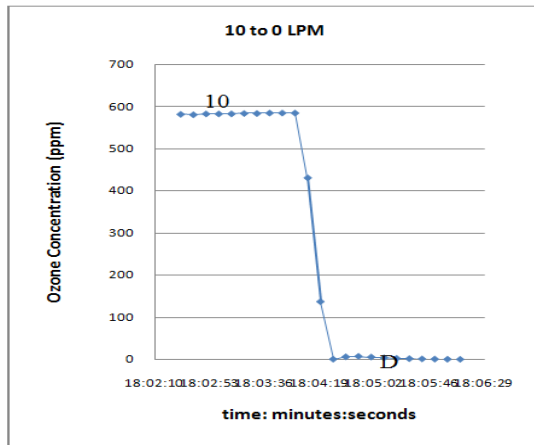


Figure 8. Effect of flow meter between $166.67 \text{ cm}^3\text{s}^{-1}$ and $0 \text{ cm}^3\text{s}^{-1}$ (10 and 0 LPM) of ozone concentrations

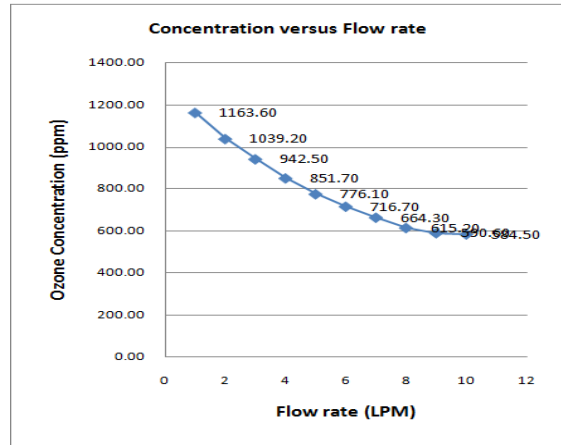


Figure 9. Effect of flow rate on ozone concentrations

Similarly, Figure 11 shows the maximum and minimum ozone concentrations in ppm obtained at an initial oxygen flow rate of $25.00 \text{ cm}^3\text{s}^{-1}$ (1 LPM). The section E is when oxygen was fed into the ozone generator while the ozone generator was off. F is the maximum ozone concentrations 4435.20 ppm at an oxygen flow rate of $25 \text{ cm}^3\text{s}^{-1}$ with the control valve completely locked to short out ozone from the destructor. G is the lowest ozone concentration obtained 387.30 ppm , when the control valve was completely opened thus allowing maximum flow of ozone to the destructor. Similarly, the percentage regulation at a flow rate of $25 \text{ cm}^3\text{s}^{-1}$ is in the range of 8.37% to 100%.

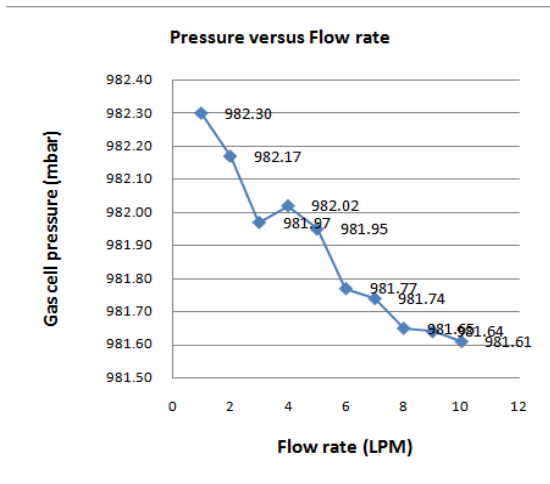


Figure 10. Effect of flow rate on the pressure of ozone gas in the gas cell

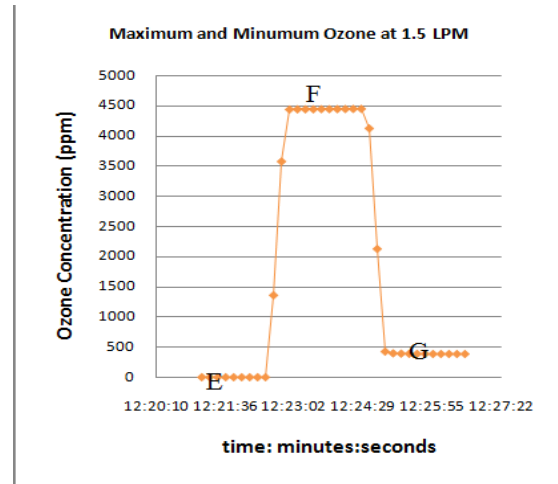


Figure 11. Maximum and Minimum ozone concentrations at an oxygen flow rate of $25.00 \text{ cm}^3\text{s}^{-1}$ (1.5 LPM)

The ozone concentration was adjusted to approximately 1000 ppm at an ozone flow rate of approximately $21.67 \text{ cm}^3\text{s}^{-1}$ (1.3 LPM). In Figure 12, 13, 14, and 15 the effect of the flow meter when the ozone was set to 1000 ppm approximately is shown. The concentrations obtained for $16.67 \text{ cm}^3\text{s}^{-1}$ to $166.67 \text{ cm}^3\text{s}^{-1}$ (1 to 10 LPM) are 1253.30, 1105.50, 976.25, 879.50, 783.50, 728.00, 663.80, 628.60, 589.00 and 563.50 ppm respectively. Similarly, the higher the flow rate the lower the concentrations, as shown in Figure 16. Figure 17 is the shows the

fluctuations in pressure at higher flow rates, at in innitial oxygen flow rate of $25\text{ cm}^3\text{s}^{-1}$ as compared $33.33\text{cm}^3\text{s}^{-1}$ the fluctuation is minimal and the gas pressure in the regulator was able to sustain a steady flow between $16.67\text{cm}^3\text{s}^{-1}$ to $150.00\text{cm}^3\text{s}^{-1}$ (1 to 9 LPM), this is shown in Figure 10, fluctuations sets in at $166.67\text{cm}^3\text{s}^{-1}$ (10 LPM). At H in Figure 15, the ozone generator is switched off and ozone concentration to reduce to approximately zero. The results are also in agreement with gas flow theory in parallel pipes.

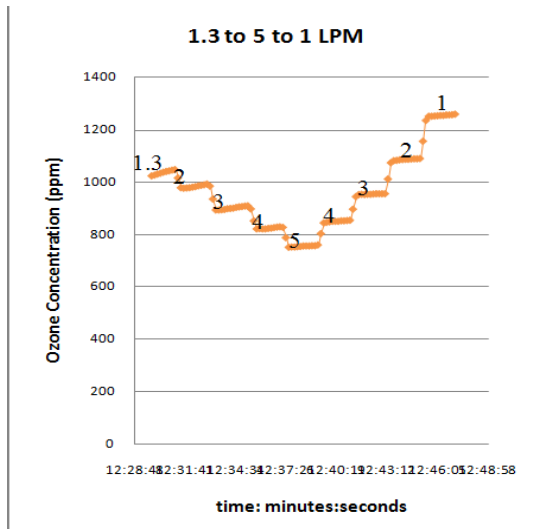


Figure 12. Effect of flow meter between $21.67\text{cm}^3\text{s}^{-1}$ to $83.33\text{ cm}^3\text{s}^{-1}$ to $16.67\text{cm}^3\text{s}^{-1}$ (1.3 to 5 to 1 LPM) of ozone concentrations

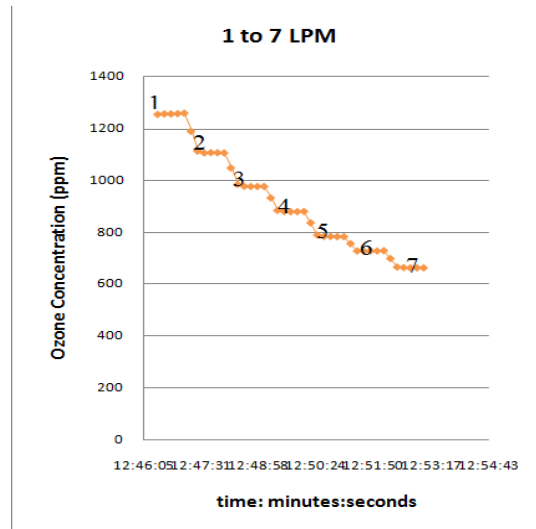


Figure 13. Effect of flow meter between $16.67\text{ cm}^3\text{s}^{-1}$ to $116.67\text{cm}^3\text{s}^{-1}$ (1 and 7 LPM) of ozone concentrations

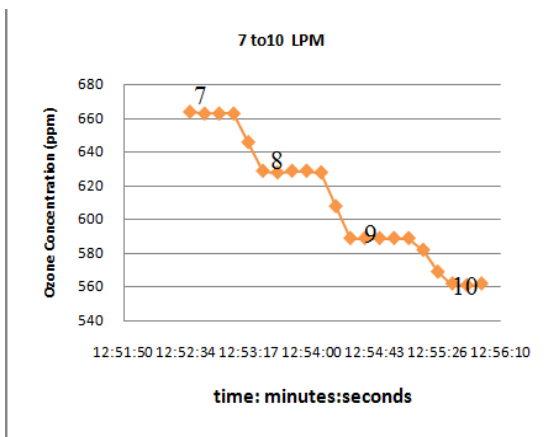


Figure 14. Effect of flow meter between $116.67\text{ cm}^3\text{s}^{-1}$ and $166.67\text{cm}^3\text{s}^{-1}$ (7 and 10 LPM) of ozone concentrations

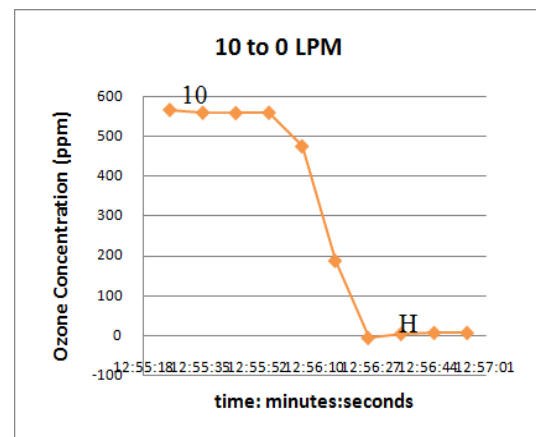


Figure 15. Effect of flow meter between $166.67\text{ cm}^3\text{s}^{-1}$ and $16.67\text{cm}^3\text{s}^{-1}$ (10 and 0 LPM) of ozone concentrations

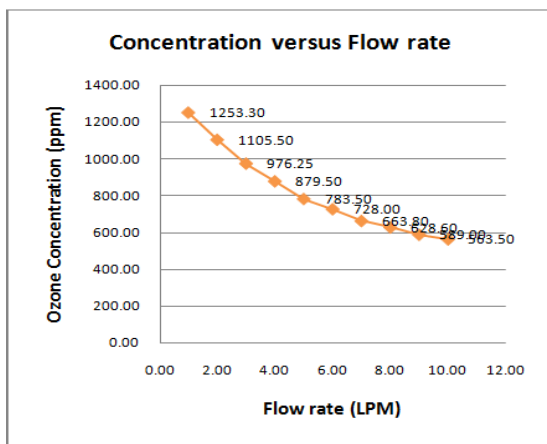


Figure 16. Effect of flow rate on ozone concentrations

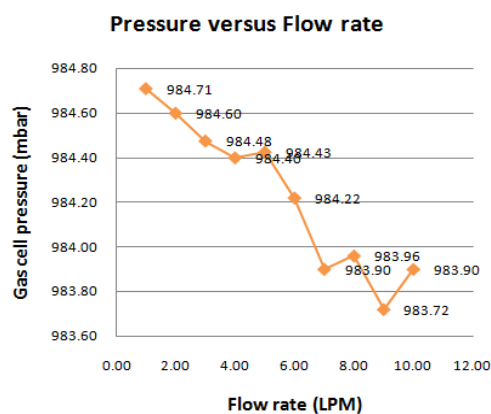


Figure 17. Effect of flow rate on the pressure of ozone gas in the gas cell

5. Conclusion

A new ozone regulator has been designed and build on the theory of continuity for gas flow in parallel pipes. The ozone regulator makes it possible to generate varying concentrations of ozone at different flow rates and thus providing for maximum flexibility in terms of concentration and flow rates. For a given flow rate varying concentrations can be obtained: at initial oxygen flow rate of $25.00 \text{ cm}^3\text{s}^{-1}$ and $33.33\text{cm}^3\text{s}^{-1}$ yields an ozone flow of $50.00 \text{ cm}^3\text{s}^{-1}$ (3 LPM) whose contraction were 976.25 ppm and 942.50 LPM respectively. Similarly a specific concentration can also be generated at different flow rates taking the advantage of the regulator: approximately 1000 ppm of ozone was generated at $21.67 \text{ cm}^3\text{s}^{-1}$ (1.3 LPM) and $30.00 \text{ cm}^3\text{s}^{-1}$ (1.8 LPM) corresponding to initial oxygen flow rate of $25.00 \text{ cm}^3\text{s}^{-1}$ and $33.33\text{cm}^3\text{s}^{-1}$ respectively. Effects of the regulator and the flow meter has also been tested and has been found to be satisfactory. The regulator has a capability of varying concentrations of ozones between 8.73% to 100%.

Acknowledgements

The authors would like to thank Universiti Teknologi Malaysia (UTM) for sponsoring this publication under Research University Grant (RUG) Scheme, grant no: 05J60 and 04H35; and Fundamental Research Grant Scheme (FRGS) grant no: 4F317 and 4F565. The Ministry of education (MOE) Malaysia is also acknowledge and the Nigerian Education Trust Fund (ETF) for the financial support giving inform of Tertiary Education Trust Fund (TET-Fund).

References

- [1] Wei LS, Yuan DK, Zhang YF, Hu ZJ, Dong GP. Experimental and theoretical study of ozone generation in pulsed positive dielectric barrier discharge. *Vacuum*. 2014; 104: 61-4.
- [2] Heleno FF, De Queiroz MEL, Neves AA, Freitas RS, Faroni LRA, De Oliveira AF. Effects of ozone fumigation treatment on the removal of residual difenoconazole from strawberries and on their quality. *Journal of Environmental Science and Health, Part B*. 2014; 49: 94-101.
- [3] Wang XD, Lv Y, Li MM, Liu HY. Removal of Nonylphenol from Water by Ozone. *Advanced Materials Research*. 2014; 859: 357-60.
- [4] Wang J, Ning FG, Yu WD. Effects of Ozone Treatment on Wool Morphology and Mechanical Properties. *Advanced Materials Research: Trans Tech Publ*. 2014; 75-8.
- [5] Raja M. Surface Modification of Carbon Nanotubes with Combined UV and Ozone Treatments. *Fullerenes, Nanotubes and Carbon Nanostructures*. 2015; 23: 11-6.
- [6] Guo WQ, Yin RL, Zhou XJ, Du JS, Cao HO, Yang SS, et al. Sulfamethoxazole degradation by ultrasound/ozone oxidation process in water: Kinetics, mechanisms, and pathways. *Ultrasonics sonochemistry*. 2015; 22: 182-7.

-
- [7] Zhang J, Zhang R, Chen X, Tong M, Kang W, Guo S, et al. Simultaneous Removal of NO and SO₂ from Flue Gas by Ozone Oxidation and NaOH Absorption. *Industrial & Engineering Chemistry Research*. 2014; 53: 6450-6.
- [8] Bertol CD, Vieira KP, Rossato LG, D'Avila JV. *Microbiological Environmental Monitoring After the Use of Air Purifier Ozone Generator*. *Ozone: Science & Engineering*. 2012; 34: 225-30.
- [9] RESOURCES L. Ext50 Ozone Generator 220/240 Volt Owners Manual And Ozone Output Test Report.
- [10] Hadji K, Pontiga F, Belasri A, Hadj-Ziane S, Fernández-Rueda A. Experimental Study of Ozone Generation by Negative Corona Discharge in Mixtures of N₂ and O₂. *Ozone: Science & Engineering* 2014; 36: 65-72.
- [11] David M, Marcus TCE, Yaacob M, Salim MR, Hussin N, Ibrahim MH, et al. Enhancement of the Response time of a Reflective Type Sensor for Ozone Measurements. *Jurnal Teknologi*. 2014; 69.
- [12] De Maria L, Bartalesi D. A fiber-optic multisensor system for predischarges detection on electrical equipment. *IEEE Sensors Journal*. 2012; 12: 207-12.
- [13] Teranishi K, Shimada Y, Shimomura N, Itoh H. Investigation of Ozone Concentration Measurement by Visible Photo Absorption Method. *Ozone: Science & Engineering*. 2013; 35: 229-39.
- [14] David M, Marcus TCE, Yaacob M, Salim MR, Ibrahim MH, Idrus SM, et al. *Sensitivity and response time of an ozone sensor*. *Photonics (ICP)*. IEEE 4th International Conference on: IEEE; 2013: 50-2.
- [15] Kumar KL. *Engineering Fluid Mechanics*. ERUSIA PUBLISHING HOUSE (P) LTD RAM NAGAR, NEW DELHI-110 055. Eight Revised Multicolour Edition: 417-23.
- [16] Çengel YA, Cimbala JM. *Fluid Mechanics Fundamentals and Applications*. Chapter 8: Flow in Pipes. Published by McGraw-Hill, a business unit of The McGraw-Hill Companies, Inc, 1221 Avenue of the Americas, New York, NY 10020 Copyright ©2006 First Edition 2006.